
Version 6.2

FitAll

nonlinear regression analysis

Peaks Function Guide

MIR
SOFTWARE

Copyright © 1984 .. 2009 by MTR Software
All rights reserved.

Published by

MTR Software

77 Carlton Street, Suite 808
Toronto ON Canada
M5B 2J7

www.fitall.com

support@fitall.com

416-596-1499

FitAll, the FitAll Function Libraries, the FitAll Getting Started Guide, the FitAll Reference Guide, the FitAll Programmer's Guide and the FitAll Function Guides are copyrighted and sold with the understanding that they will be used either on a single computer or by one individual, whichever is most appropriate for the purchaser.

When you purchase FitAll, you purchase a SINGLE USER LICENCE.

Selling (or giving) copies of FitAll, its Function Libraries or Guides to others is an infringement of the copyright. That means it is illegal!.

"FitAll" and "fitting solutions" are trade marks of MTR Software.

Contents

Introduction	1
Function Reference	3
Ftn 0301: Gaussian With Background Correction.....	4
Ftn 0302: Sum of Gaussians With Background Correction.....	6
Ftn 0303: Lorentzian With Background Correction.....	9
Ftn 0304: Sum of Lorentzians With Background Correction.....	11
Ftn 0305: Sum of Gaussians and Lorentzians With Background Correction	14
Ftn 0306: Poisson With Background Correction.....	16
Ftn 0307: Impulse: Linear or Exponential Growth Coupled with Exponential Decay	18
Appendix	21
Getting Help.....	22
Adding Functions to FitAll.....	23
Index	25

Introduction

This **FitAll™ Peaks Function Guide** describes the functions contained in the **Peak Functions Library** and has an appendix that explains how to get help from **MTR Software**.

[Function Reference](#) ³

[Appendix](#) ²¹

Function Reference

Overview

This section describes each of the functions in *FitAll's Peak Functions Library*.

In most cases, a graph of the function is shown. These graphs were created using "typical" parameter and constant values.

The actual appearance of a function depends on the parameter and constant values and may look quite different from the illustrations shown.

Equation

Gives the equation and its variations. The variations are listed in order of increasing complexity.

Constants

Lists the constants, K, that are used in the function. The default values for the constants also are given.

Parameters

Lists the parameters, P, that are used in the function.

Multi-Fits

Describes the Multi-Fit functionality of "Multi-Fit enabled" functions.

Sample Applications

Gives examples of some situations in which the function is known to be used.


Remarks

Provides general comments and hints, and lists any known limitations or restrictions that should be observed when using the function.

Also see

Provides links or references to other related functions.

Ftn 0301: Gaussian With Background Correction

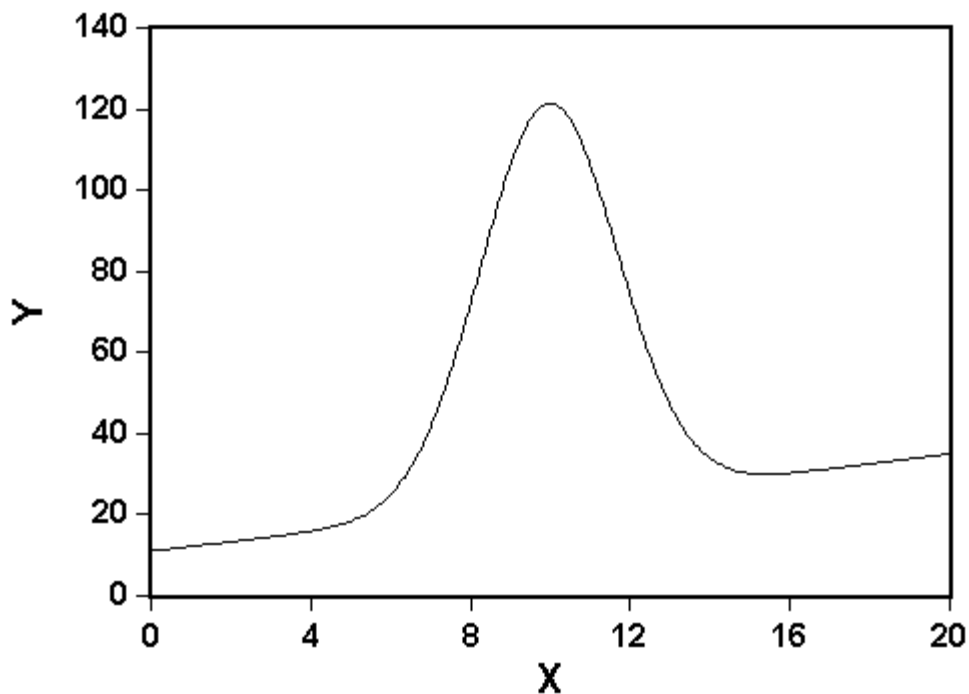

Equation

$$Y = P1 * e^{-2.77 * \left(\frac{(X - P2)}{P3}\right)^2} + \sum_{i=0} A_i * X^i$$

Four variations of the function are available, for example:

$$\bullet Y = P1 * e^{-2.77 * \left(\frac{(X - P2)}{P3}\right)^2}$$

$$\bullet Y = P1 * e^{-2.77 * \left(\frac{(X - P2)}{P3}\right)^2} + P4 + P5 * X$$

in which:

- Y is the measured response.
- X is the independent variable, often the concentration of a substance.

Parameters

Parameter	Name	Comments
P1	Ypeak	Maximum value of Y.
P2	Xpeak	Value of X when Y = Ypeak.
P3	FWHH	Full-Width at Half-Height. Width of the curve at Y = Ypeak/2.
P4	A0	Constant background offset.
P5	A1	Linear background correction term.
P6	A2	Quadratic background correction term.


Sample Applications

- Fitting adsorption or emission peaks.
- Fitting chromatographic peaks.

Remarks

When automatic initial estimates are made, **FitAll** assumes that the data are sorted on column number 1; that is, the X-values.

Ftn 0302: Sum of Gaussians With Background Correction

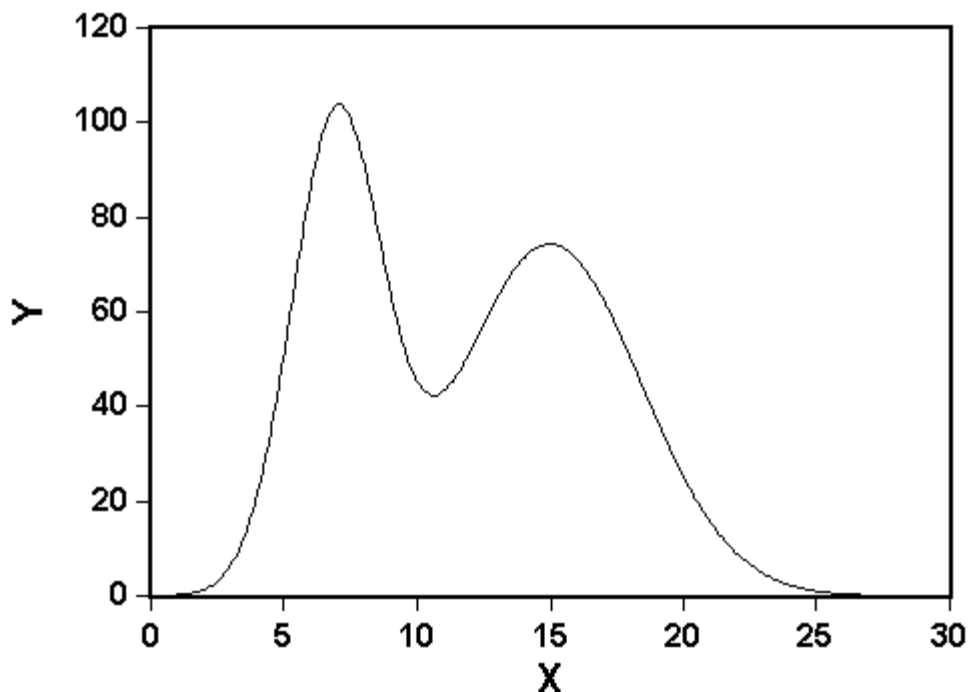

Equation

The general form of the function is:

$$Y = \sum_{i=1}^n \left[P_{3i-2} * e^{\left[-2.77 * \left(\frac{X - P_{3i-1}}{P_{3i}} \right)^2 \right]} \right] + \sum_{j=0}^{n2} \left(P_{3n+1+j} * X^j \right)$$

in which:

- Y is the measured response.
- X is the independent variable, often the concentration of a substance.

For example:

$$Y = P_1 * e^{\left[-2.77 * \left(\frac{X - P_2}{P_3} \right)^2 \right]}$$

$$Y = P1 * e^{\left[-2.77 * \left(\frac{X - P2}{P3}\right)^2\right]} + P4 + P5 * X + P6 * X^2$$

$$Y = P1 * e^{\left[-2.77 * \left(\frac{X - P2}{P3}\right)^2\right]} + P4 * e^{\left[-2.77 * \left(\frac{X - P5}{P6}\right)^2\right]}$$

$$Y = P1 * e^{\left[-2.77 * \left(\frac{X - P2}{P3}\right)^2\right]} + P4 * e^{\left[-2.77 * \left(\frac{X - P5}{P6}\right)^2\right]} +$$

$$P7 * e^{\left[-2.77 * \left(\frac{X - P8}{P9}\right)^2\right]}$$

Parameters

Parameter	Name	Comments
P1	Ypeak1	Maximum value of Y for the first Gaussian curve.
P2	Xpeak1	Value of X when Y = Ypeak1.
P3	FWHH1	Full-Width at Half-Height for the first Gaussian curve. Width of the curve at Y = Ypeak1/2.
P4	Ypeak2	Maximum value of Y for the second Gaussian curve.
P5	Xpeak2	Value of X when Y = Ypeak2.
P6	FWHH2	Full-Width at Half-Height for the second Gaussian curve. Width of the curve at Y = Ypeak2/2.
P7	Ypeak3	Maximum value of Y for the second Gaussian curve.
etc.	etc.	etc.
	A0	Constant background offset.
	A1	Linear background correction term.
	A2	Quadratic background correction term.

Sample Applications

- Fitting adsorption or emission peaks.
- Fitting chromatographic peaks.


Remarks

When automatic initial estimates are made, **FitAll** assumes that the data are sorted on column number 1; that is, the X-values.

FitAll will calculate initial estimates only when you are fitting the data to one Gaussian.

Often the best fitting strategy is to fit only part of your data to one Gaussian curve, then fit a larger segment of the data to the sum of two Gaussians, etc., until all of your data are included in the analysis.

Ftn 0303: Lorentzian With Background Correction

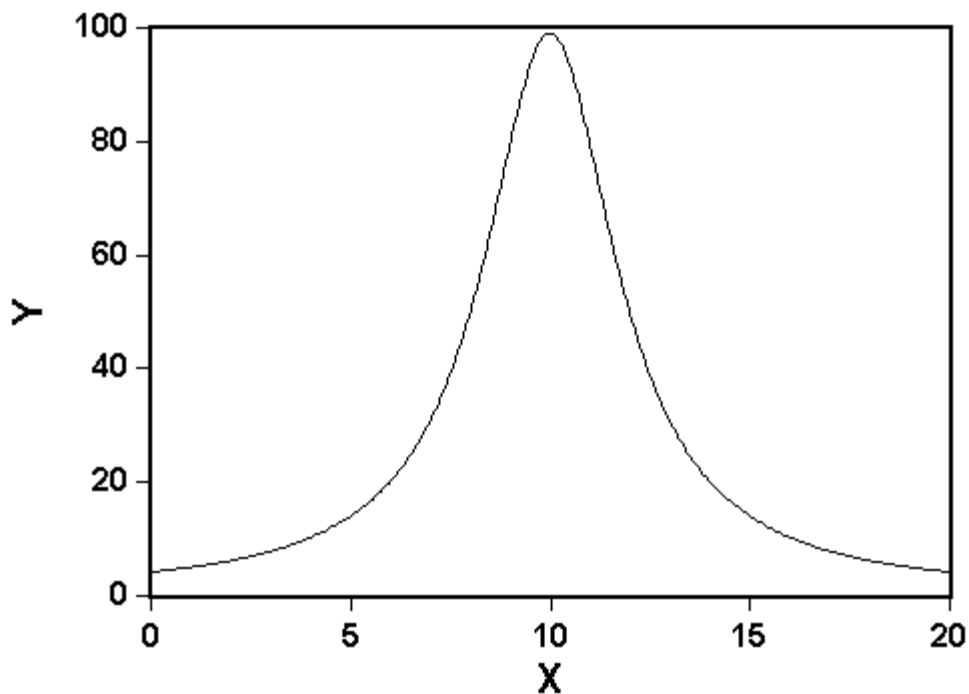

Equation

$$Y = \frac{P1 * P3^2}{\left[4 * (X - P2)^2 + P3^2 \right]} + \sum_i A_i * X^i$$

For example:

$$Y = \frac{P1 * P3^2}{\left[4 * (X - P2)^2 + P3^2 \right]}$$

$$Y = \frac{P1 * P3^2}{\left[4 * (X - P2)^2 + P3^2 \right]} + P4 + P5 * X$$

in which:

- Y is the measured response.
- X is the independent variable, often the time or concentration of a substance.

Parameters

Parameter	Name	Comments
P1	Ypeak	Maximum value of Y.
P2	Xpeak	Maximum value of Y.
P3	FWHH	Full-Width at Half-Height. Width of the curve at $Y = Y_{\text{peak}}/2$.
P4	A0	Constant background offset.
P5	A1	Linear background correction term.
P6	A2	Quadratic background correction term.


Sample Applications

- Fitting adsorption or emission peaks.

Remarks

When automatic initial estimates are made, **FitAll** assumes that the data are sorted on column number 1; that is, the X-values.

Ftn 0304: Sum of Lorentzians With Background Correction

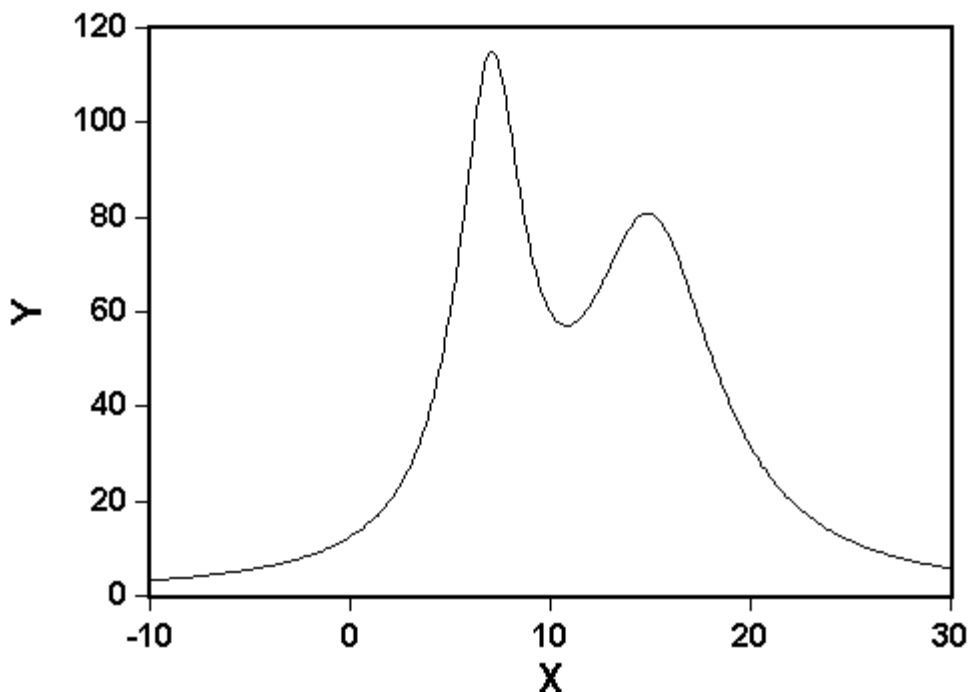

Equation

The general form of the function is:

$$Y = \sum_{i=1}^n \left(\frac{P_{3i-2} * P_{3i}^2}{4 * (X - P_{3i-1})^2 + P_{3i}^2} \right) + \sum_{j=0}^{n2} (P_{3n+1+j} * X^j)$$

in which:

- Y is the measured response.
- X is the independent variable, often the time in seconds.

For example:

$$Y = \frac{P1 * P3^2}{4 * (X - P2)^2 + P3^2}$$

$$Y = \frac{P1 * P3^2}{4 * (X - P2)^2 + P3^2} + P4 + P5 * X + P6 * X^2$$

$$Y = \frac{P1 * P3^2}{[4 * (X - P2)^2 + P3^2]} + \frac{P4 * P6^2}{[4 * (X - P5)^2 + P6^2]}$$

Parameters

Parameter	Name	Comments
P1	Ypeak1	Maximum value of Y for the first Lorentzian curve.
P2	Xpeak1	Value of X when Y = Ypeak1.
P3	FWHH1	Full-Width at Half-Height for the first Lorentzian curve. Width of the curve at Y = Ypeak1/2.
P4	Ypeak2	Maximum value of Y for the second Lorentzian curve.
P5	Xpeak2	Value of X when Y = Ypeak2.
P6	FWHH2	Full-Width at Half-Height for the second Lorentzian curve. Width of the curve at Y = Ypeak2/2.
P7	Ypeak3	Maximum value of Y for the second Lorentzian curve.
etc.	etc.	etc.
	A0	Constant background offset.
	A1	Linear background correction term.
	A2	Quadratic background correction term.

Sample Applications

- Fitting adsorption or emission peaks.
- Fitting chromatographic peaks.

Remarks


When automatic initial estimates are made, **FitAll** assumes that the data are sorted on column number 1; that is, the X-values.

FitAll will calculate initial estimates only when you are fitting the data to one Lorentzian.

Often the best fitting strategy is to fit only part of your data to one Lorentzian curve, then fit a larger

segment of the data to the sum of two Lorentzians, etc., until all of your data are included in the analysis.

Ftn 0305: Sum of Gaussians and Lorentzians With Background Correction

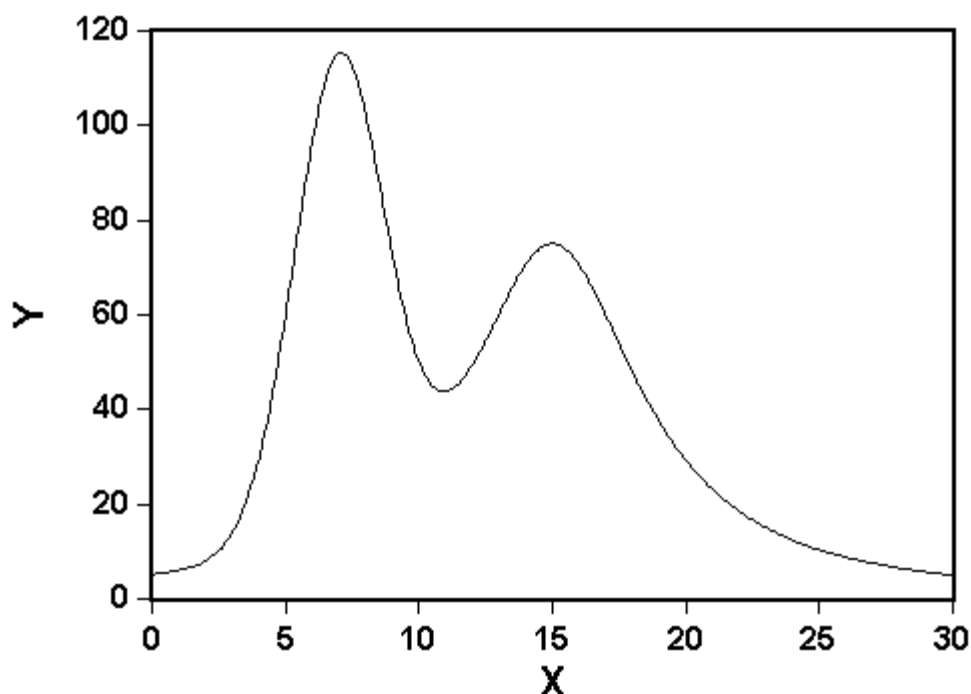

Equation

Y is the sum of one to five Gaussian and Lorentzian curves. That is, the total number of Gaussians plus Lorentzians is limited to five.

The simplest form of the function is:

$$Y = P1 * e^{\left[-2.77 * \left(\frac{X - P2}{P3} \right)^2 \right]} + \frac{P4 * P6^2}{[4 * (X - P5)^2 + P6^2]}$$

in which:

- Y is the measured response.
- X is the independent variable.
- All forms of the above may also have a background correction polynomial of up to three terms, that is, a quadratic polynomial.

Parameters

Parameter	Name	Comments
P1	YpeakG1	Maximum value of Y for the first Gaussian curve.
P2	XpeakG1	Value of X when Y = YpeakG1.
P3	FWHHG1	Full-Width at Half-Height for the first Gaussian curve. Width of the curve at $Y = Y_{peak1} / 2$.
P4	YpeakL1	Maximum value of Y for the first Lorentzian curve.
P5	XpeakL1	Value of X when Y = YpeakL1.
P6	FWHHL1	Full-Width at Half-Height for the first Lorentzian curve. Width of the curve at $Y = Y_{peakL1} / 2$.
P7	Ypeak3	Maximum value of Y for the second Lorentzian curve.
etc.	etc.	etc.
	A0	Constant background offset.
	A1	Linear background correction term.
	A2	Quadratic background correction term.

Sample Applications

- Fitting adsorption or emission peaks.
- Fitting chromatographic peaks.

Remarks


When automatic initial estimates are made, **FitAll** assumes that the data are sorted on column number 1; that is, the X-values.

FitAll will calculate only some of the required initial estimates - those for the first Gaussian and the background polynomial correction terms.

FitAll assumes that the first part of the data will correspond to the first Gaussian rather than to the first Lorentzian. The remaining initial parameter estimates must be entered manually.

Often the best fitting strategy is to fit only part of your data to one Gaussian curve or to one Lorentzian curve, then fit a larger segment of the data to the sum of two Gaussians, etc., until all of your data are included in the analysis.

Ftn 0306: Poisson With Background Correction

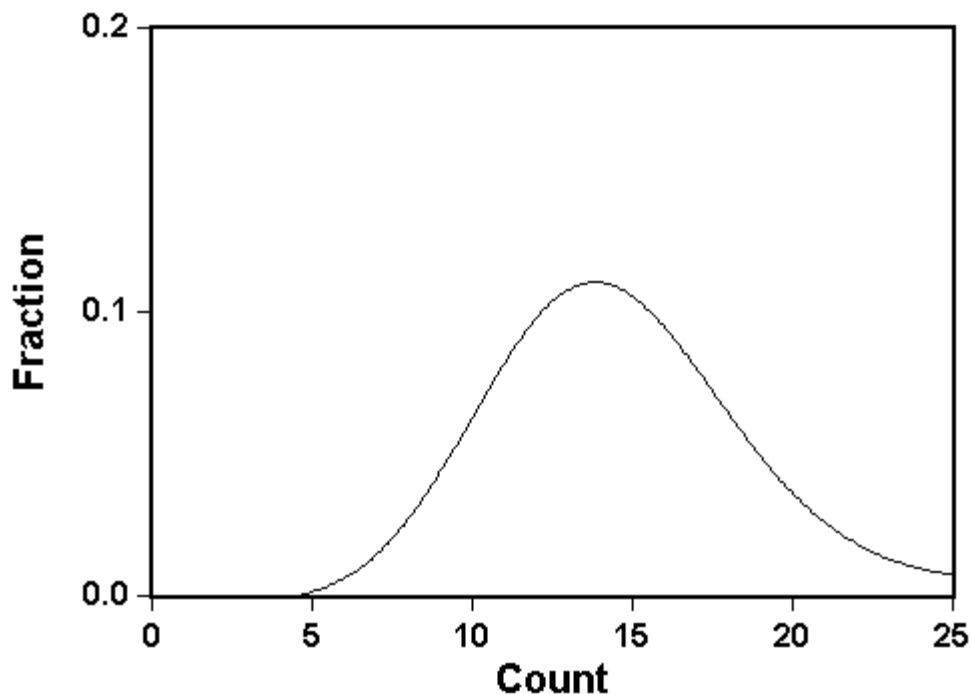

Equation

$$Y = P2 * e^{[X * \text{Ln}(P1) - P1 - \text{Ln}(X!)]} + \sum_{i=0}^n (A_i * X^i)$$

For example:

- $Y = P2 * e^{[X * \text{Ln}(P1) - P1 - \text{Ln}(X!)]}$

- $Y = P2 * e^{[X * \text{Ln}(P1) - P1 - \text{Ln}(X!)]} + P3 + P4 * X$

in which:

- Y is the measured response.
- X is the independent variable.

Parameters

Parameter	Name	Comments
P1	Xmean	Mean (average) value of the Poisson distribution. The standard deviation of a Poisson distribution is


Parameter	Name	Comments
		equal to the square root of the mean.
P2	NF	Normalization Factor. Amplitude scaling factor, such that $\text{Sum}\{Y_i\}/P2 = 1.0$. If the Y-values correspond to the probability of observing X events per unit time, P2 should have a value of 1.
P3	A0	Constant background offset.
P4	A1	Linear background correction term.
P5	A2	Quadratic background correction term.

Remarks

All X-values must be greater than or equal to one ($X \geq 1$).

When automatic initial estimates are made, **FitAll** assumes that the data are sorted on column number 1, that is, the X-values.

Ftn 0307: Impulse: Linear or Exponential Growth Coupled with Exponential Decay

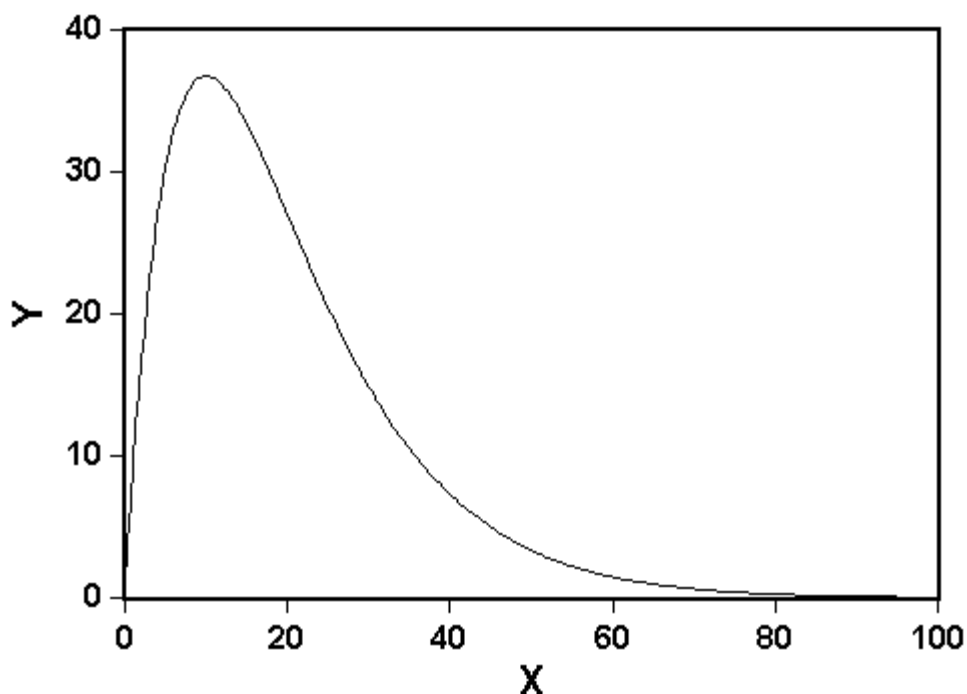

Equation

The general form of the function is:

$$Y = P1 * (X - P3)^{P4} * e^{-P2 * K1 * (X - P3)} + \sum_{i=0}^n (A_i * X^i)$$

For example:

$$\bullet Y = P1 * X * e^{-P2 * K1 * X}$$

$$\bullet Y = P1 * (X - P3) * e^{-P2 * K1 * (X - P3)}$$

$$\bullet Y = P1 * (X - P3)^{P4} * e^{-P2 * K1 * (X - P3)}$$

in which:

- Y is the measured response.
- X is the independent variable, often the time in seconds.

Constants

Constant	Name	Comments
K1	K1	Arbitrary constant. Default value is 1.0.

Parameters

Parameter	Name	Comments
P1	P1	Amplitude of the exponential term.
P2	P2	Rate constant or 1/(time constant) for the exponential decay.
P3	P3	X offset (time zero offset). In the first two forms of the function P3 is assumed to be zero.
P4	P4	Growth order parameter. In the first two functions P4 is 1.0; that is, first order growth is assumed.
	A0	Constant background offset.
	A1	Linear background correction term.
	A2	Quadratic background correction term.

Sample Applications

- Describes an "impulse", such as that encountered when adding a "slug" of reagent to a chemical reactor in which mixing is not instantaneous.
- Describes the uptake and release of nutrients by biological systems.

Remarks

In the third form of the function, (X-P3) is assumed to be greater than zero (> 0).

When automatic initial estimates are made, **FitAll** assumes that the data are sorted on column number 1; that is, the X-values.

Appendix

[Getting Help](#)  22

[Adding Functions to FitAll](#)  23

Getting Help

To get technical or other assistance from MTR Software you can:

Visit the FAQ page on MTR Software's web site at:

www.fitall.com

Email MTR Software at:

support@fitall.com

Write to MTR Software at:

MTR Software

77 Carlton Street, Suite 808

Toronto ON Canada

M5B 2J7

Telephone MTR Software at:

416-596-1499

Describe your problem or difficulty as completely as you can. We will try to answer your query quickly and completely.

You should also include your email address as well as your daytime, evening and weekend telephone numbers.

Adding Functions to FitAll

There are three ways to add your own specialized functions to *FitAll*.

1. You can contact **MTR Software** to get a quotation on the cost of creating a custom **FitAll Function Library** for you.
2. The *FitAll* Programmer's Guide, which is included with **FitAll Research Edition**, explains:
 - how to modify the supplied source code for the User Defined **FitAll Function Libraries** and
 - how to compile them using Borland Delphi version 5, 6, 7, 2005 and 2006.
3. You can contact **MTR Software** and request that the function be added to one of *FitAll's* **Function Libraries**.

Index

sum of 11, 14

- P -

Poisson 16

- A -

Adding Functions to FitAll 23

- C -

Contacting MTR Software 22

- E -

Exponential 18
Gaussian 4
Impulse 18
sum of Gaussians 6
sum of Gaussians and Lorentzians 14

- F -

Function 4, 6, 9, 11, 14, 16, 18
adding to FitAll 23
Function Reference 3

- G -

Gaussian 4
sum of 6, 14

- H -

Help 22
How to
contact MTR Software 22

- I -

Impulse 18

- L -

Lorentzian 9